

TEST REPORT

(Electronic version)



No:200104365

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: OFBG-7901-34

ISSUE DATE:2020-04-29

检测报告



APPLICANT: DONGGUAN FORES BIOTECHNOLOGY CO., LTD
ADDRESS: ROOM 201, NO. 1 BUILDING, NO. 5, SHIPAI INDUSTRIAL AVENUE, SHIPAI TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

INFORMATION CONFIRMED BY APPLICANT:

KN95 PROTECTIVE MASK

QUANTITY: EIGHTY PIECES

MANUFACTURE'S NAME: DONGGUAN FORES BIOTECHNOLOGY CO., LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-29

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200068920.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

Yuan Liu ENGINEER

刘圆




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200104365

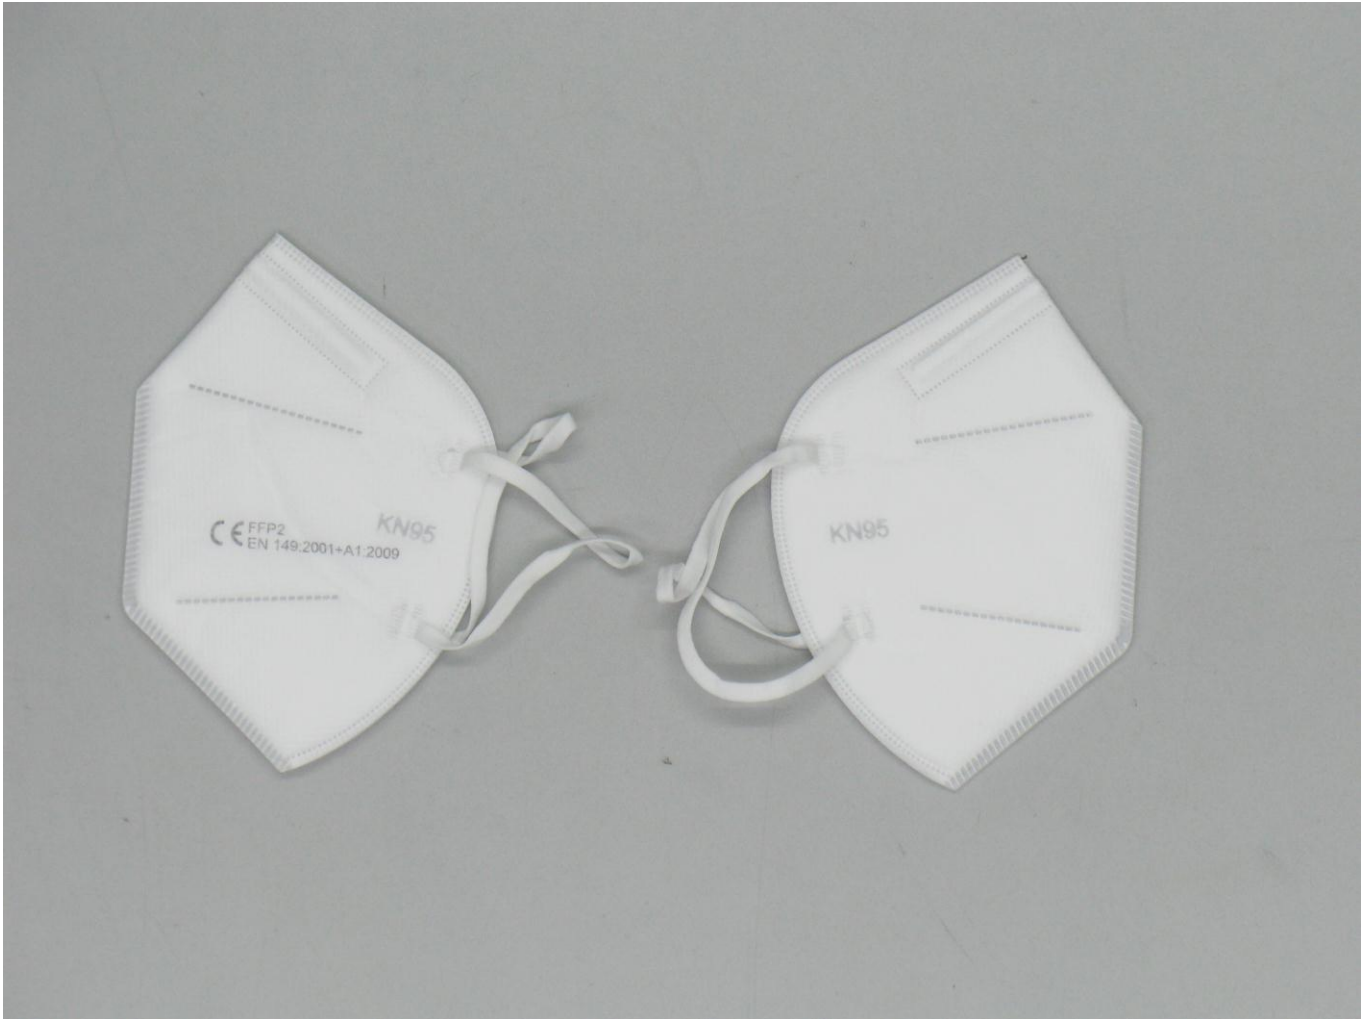

TEST REPORT

(Electronic version)

No:200104365

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION, 15mg/m³,
TEMP:23.6℃ RH:35.4%)

FILTRATION EFFICIENCY(%) :

UNTREATED SAMPLE

1# 95.87
2# 95.76
3# 96.14
4# 95.90
5# 95.82
6# 95.48
7# 96.27
8# 96.11
9# 95.49
10# 95.79

CONDITIONING TREATED

1# 96.98
2# 95.79
3# 95.36
4# 96.11
5# 95.90

REQUIREMENT

FILTRATION EFFICIENCY(%) :

≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 135.4
2# 137.3

PRETREATMENT SAMPLE:

1# 125.5
2# 128.3

REQUIREMENT

≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 121.8
2# 127.9

PRETREATMENT SAMPLE:

1# 107.4
2# 112.6

REQUIREMENT

≤250
(GB 2626-2006)

FLAMMABILITY (s)

(GB 2626-2006 6.15)

AFTERFLAME TIME

UNTREATED SAMPLE

1# 0.0
2# 0.0

CONDITIONING TREATED

3# 0.0
4# 0.0

REQUIREMENT

AFTERFLAME TIME
≤5
(GB 2626-2006)



PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200104365

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST

PARTS OF MASK SHOULD NOT SLIP OR BREAK

UNDER 10N TENSION FOR 10S.

(GB 2626-2006)



—End of Report—

PAGE 4 OF 4