

TEST REPORT

(Electronic version)



No: 200093459

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: QDCR-6619-34

ISSUE DATE: 2020-04-26

检测报告



APPLICANT: DONGGUAN FORES BIOTECHNOLOGY CO., LTD
ADDRESS: ROOM 201, NO. 1 BUILDING, NO. 5, SHIPAI INDUSTRIAL AVENUE, SHIPAI TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

INFORMATION CONFIRMED BY APPLICANT:

DISPOSABLE FACE MASK

QUANTITY: TWENTY PIECES

MANUFACTURE'S NAME: DONGGUAN FORES BIOTECHNOLOGY CO., LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-24

CONCLUSION:

PARTICLE FILTRATION EFFICIENCY M

AIRFLOW RESISTANCE M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THE DECISION INDICATORS ARE DERIVED FROM THE GROUP STANDARD REQUIRED BY CLIENT (T/GDBX 025-2020). OUR INSPECTION CAPACITY AUTHORIZED BY CMA COVERS THE INSPECTION ITEMS T/GDBX 025-2020.
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200072957.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 3

TEST REPORT

(Electronic version)

No:200093459

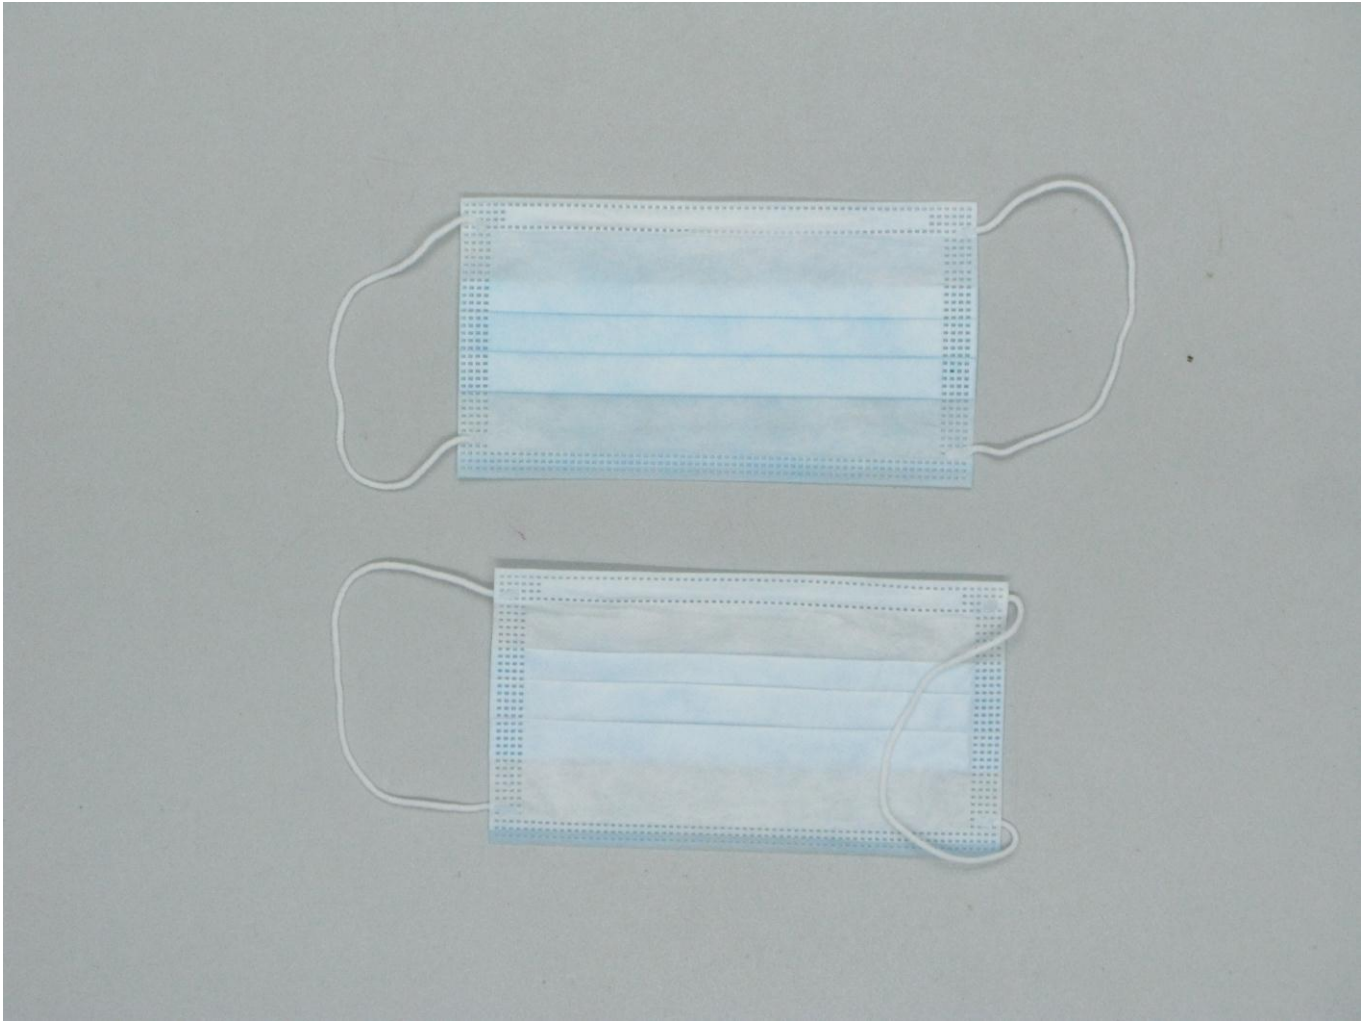

TEST REPORT

(Electronic version)

No:200093459

PARTICLE FILTRATION EFFICIENCY (%)

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 23.1°C, RH: 36.0%)

MINIMUM 81.2

REQUIREMENT

≥50

(GRADE A)

(T/GDBX 025-2020)

AIRFLOW RESISTANCE (Pa)

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 23.1°C, RH: 36.0%)

MAXIMUM 28.3

REQUIREMENT

≤70

(T/GDBX 025-2020)



—End of Report—

PAGE 3 OF 3